




CALIBRATION CERTIFICATE

DAFCHGX002140002

1 3
Page 1 of 3 Pages



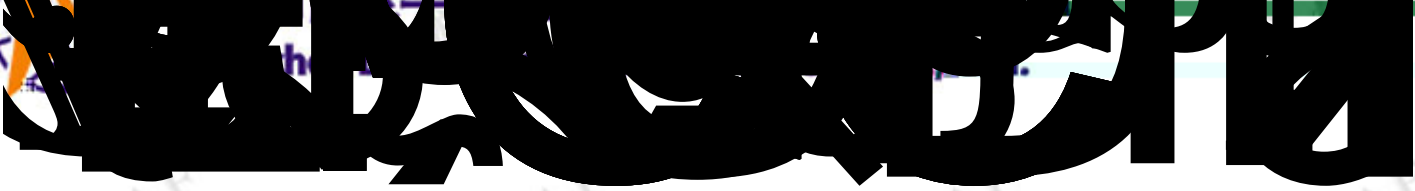

DIRECTIONS OF CALIBRATION

DAFCHGX002140002

Certificate No.

2 3
Page 2 of 3 Pages

1. The results of NLR M 1K P`





Result of Calibration

DAFCHGX002140002

3 , 3

Report No.

Page 3 of 3 Pages

1 (Appearance & Interaction)

(Normal)

2 (Detection indication error):

(Conclusion)

(Pass/Fail)

| | mg/L) | mg/L) | %) | Limit |
|-----------------|-------|-------|------|-------|
| Detection value | 10 | 10.15 | 1.5 | ±10% |
| | 50 | 50.81 | 1.6 | ± 10% |
| | 80 | 78.58 | -1.8 | ± 10% |

P

P

P

3 (Repeatability of detection):

(Conclusion)

(Pass/Fail)

| Standard value | Repeatability | Limit |
|----------------|---------------|-------|
| mg/L | % | % |
| 50 | 1.5 | 3 |

P

Notes

(Directions of measurement uncertainty in the calibration)

1. JJF1059.1-2012

(Reference Document JJF1059.1-2012 Evaluation and Expression of Uncertainty in Measurement)

2. (The expanded uncertainty of the measurement) $rel=3.2\% \quad =2$

(The below is blank)

